apple dental LABORATORY

O.H.P.A. ORALHEALTH PROFESSIONALS ASSOCIATION ACCREDITED LABORATORY

44 North Lake Road, Alfred Cove WA 6154
Phone. (08) 9329 9992
Fax. (08) 9329 9294
info@appledentallab.com.au
www.appledentallab.com.au

Surgery: _____ **Dentist:** _____

Patients Name: _____ **Sex:** ❑ M ❑ F | **Age:** _____

crown / bridge / implants

RESTORATION TYPE
- ❑ PFM
- ❑ FGC
- ❑ Post & Core
- ❑ Implant Screw Retained
- ❑ Implant Cement Retained
- ❑ Implant Brand _____

MATERIAL TYPE

Metal-Free
- ❑ applelite (Super Transluscent Zirconia)
- ❑ appleopal (Transluscent Zirconia)
- ❑ Zirconia Layered
- ❑ Inlay / Onlay
- ❑ e-max Crown
- ❑ e-max Veneer

Occlusal Contact
❑ Heavy ❑ Light ❑ Open

Proximal Contact
❑ Normal ❑ Broad

Metal
- ❑ Non-precious
- ❑ Semi-precious
- ❑ Precious (Yellow Gold)
- ❑ Other _____



Shade:
Stump Shade:
Tooth Number(s):

INSTRUCTIONS

_____
_____
_____
_____
_____

_____
_____
_____

Further Instructions PTO

apple planning

- ❑ **Implant stent**
- ❑ **Radio opaque implant stent**
- ❑ **3D Virtual stent**
- ❑ **CBCT Scan**

_____
_____
_____
_____
_____

COPING TYPE

Metal-Free
- ❑ 180° Porcelain Margin
- ❑ Full 360° Porcelain Margin
- ❑ Full 360° Metal Margin

IF INSUFFICIENT ROOM
- ❑ Reduce prep & mark model
- ❑ Reduce opposing & mark model
- ❑ Reduce prep, make reduction key
- ❑ Send back for re-prep

Email photos and files with Dr and Patient Name in the subject line to:
images@appledentallab.com.au

❑ Photos Sent

dentures

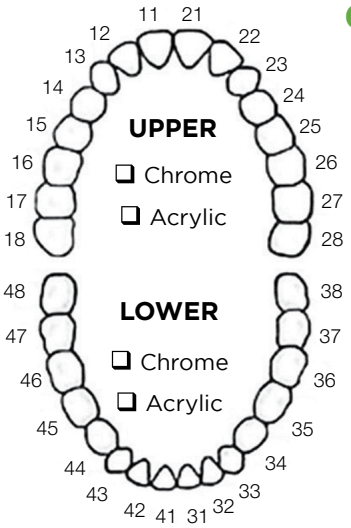

Procedure	Date/Time
❑ U ❑ L Study Models	
❑ U ❑ L Special Tray	
❑ U ❑ L Bite Block	
❑ U ❑ L Try-in	
❑ U ❑ L Retry	
❑ U ❑ L Insert	

VITA
Denture
Shade:

valplast International Corp

❑ U ❑ L Valplast	

Repairs/Relines and Additions:

_____
_____
_____

Date/Time: _____

thermoplastic CLEARsplint™ THE NIGHTGUARD WITH FLEX! splint

Splints: ❑ Upper ❑ Lower Date/Time: _____

Function: ❑ Ant Guidance ❑ Canine Guidance
❑ Night Guard (Flat Plane)

Instructions:

_____
_____

- ❑ MDSA (Anti Snore Appliance) Date/Time _____
- ❑ Suspension Bridge ❑ U ❑ L Date/Time _____
- ❑ Trutane Stent ❑ U ❑ L Date/Time _____
- ❑ Bleaching trays ❑ U ❑ L Date/Time _____

mouthguards (Colour Chart PTO)

Colour: _____ Date/Time_____

Briteguard THERMOFORMING MATERIALS | AUSTRALIA'S WORLD CLASS MOUTHGUARD MATERIAL

SINGLE COLOURS

PEARL COLOURS | FLUORESCENT COLOURS | DESIGNER COLOURS

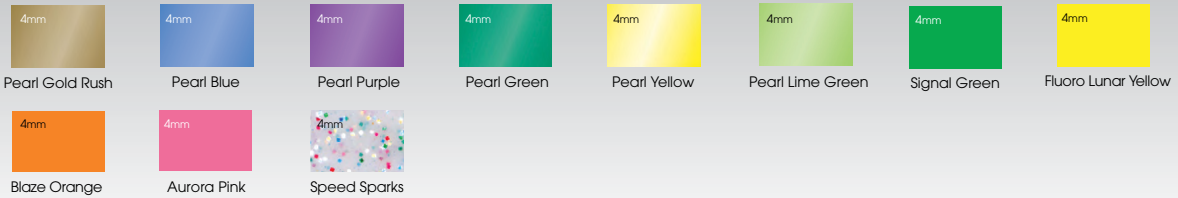

2 COLOUR | 3 COLOUR

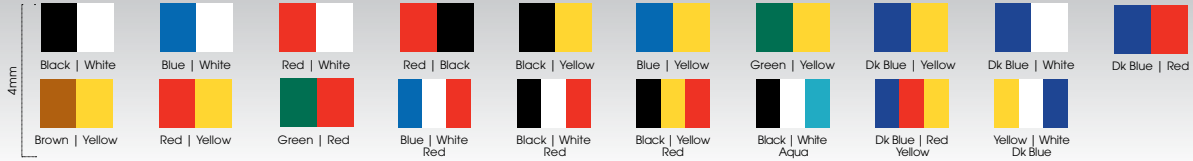

3 STRIPES | MULTI STRIPES

ALL COLOURS PRINTED ARE CLOSEST POSSIBLE MATCH TO MATERIAL COLOURS.

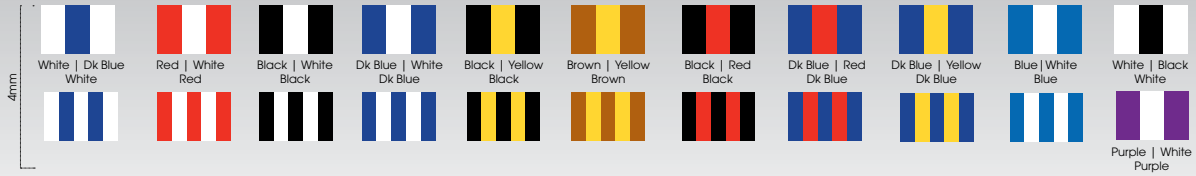

in lab working times

Soft Reline	2 working days	Splints	5 working days
Special Trays	3 working days	Implant Stents & Guides	5 working days
Bite Blocks	3 working days	Valplast Additions	2 working days
Bleaching Trays	3 working days	Valplast Process	10 working days
Mouthguards	3 working days	Crown & Bridge	10 working days
Denture Try-ins	5 working days	Chrome Castings	10 working days
Denture Inserts	5 working days		

apple dental LABORATORY

Further Instructions

CLEARsplint™ THE NIGHTGUARD WITH FLEX!

IPS e.max®

valplast International Corp

Briteguard THERMOFORMING MATERIALS

Nobel Biocare®

VITA